

COMPANY NAME : BAYRAKTAR YATIRIM İÇ VE DIŞ TİCARET A.Ş.
Firma Adı

ADDRESS : ALTINTEPSİ MAH. YAHYA KEMAL CAD. A-2 KULE NO: 112
Adresi BAYRAMPAŞA - İSTANBUL / TÜRKİYE

TEST NAME : Skin Irritation Test
Testin Adı

TEST STANDART : ISO 10993-10
Test Standardı

LOT NUMBER : 01264712
Lot Numarası:

COMMERICAL BRAND (If You Have) : Sogi-Gloves
Ticari Markası (Eğer Varsa)

NAME OF THE PRODUCT: Sogi-Gloves Powder Free Nitrile Examination Gloves
Ürünün Adı

REPORT NUMBER: 2020-11/BİYO/1-1327
Rapor Numarası

M E D I C E R T

BIOCOMPATIBILITY TEST RESPONSIBLE


Vet. Hekim Simge GARLI



MEDİCERT ULUSLARARASI ÜRÜN VE SİSTEM
BELGELENDİRME BAĞIMSIZ DENETİM
VE EĞİTİM HİZMETLERİ LTD. ŞTİ.
Tersane Mah. Cemal Gürsel Cad. No: 11/3
Halide Hanım Apt. Karşıyaka / İZMİR
Tel: 0232 327 33 44 Fax: 0232 327 33 45
Karşıyaka V.D: 613 073 9815

REPORT INDEX

COVER	: 1
INDEX	: 2
SUMMARY	: 3
INTRODUCTION	: 4
SAMPLE INFORMATION	: 4
TEST SYSTEM	: 5
ANIMAL MANAGEMENT	: 5
METHOD	: 6
EVALUATION	: 7 - 8 - 9
RESULT	: 9
RECORD	: 9
REFERENCES	: 9

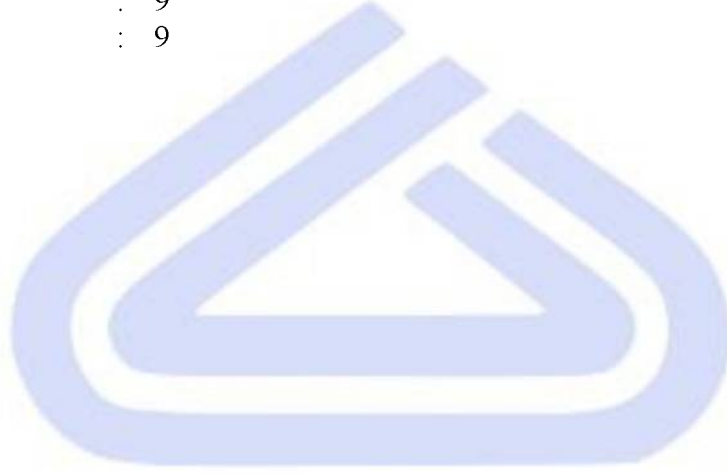

M E D I C E R T

SUMMARY:

Sogi-Gloves Powder Free Nitrile Examination Gloves sample numbered 01264712 has been subjected to a biocompatibility test according to TS EN ISO 10993-10 Biological evaluation of medical devices - Part 10: Tests for irritation and skin sensitivity. Samples were prepared by storing 37°C-72 hours in ; Serum Physiological liquid under sterile conditions according to TS EN ISO 10993-12 Biological evaluation of medical devices - Part 12: Sample preparation and reference materials standard. As a Positive Control; Sodium lauryl sulfate (SLS), previously known to have an irritant effect. As Negative Control; Serum Physiological previously known to have no irritant effect. Three rabbits were used in the study. The observation period was carried out between 10.11.2020 - 12.11.2020. The presence and absence of edema and erythema were recorded by application of the samples to the skin. The negative control was also analyzed at the same time. As a result, it was determined that the test sample did not cause any skin irritation.

M E D I C E R T

1.INTRODUCTION

Purpose : In the report described below, the potential of a single topical application for the rabbit skin irritation assay was evaluated.

Test Guide : This study was conducted according to the requirements of the International Organization for Standardization. 10993: Biological Assessment of Medical Devices, Part 10: Tests for Irritation and Skin Sensitivity

Dates

Sample Acceptance Date : 06.11.2020

Test Date : 10.11.2020

Observation Date : 12.11.2020

2. SAMPLE INFORMATION

Company Name : Bayraktar Yatırım İç Ve Dış Ticaret A.Ş.

Date of the Sample Acceptance : 06.11.2020 14:00

Sample Record Number : BYSG0006/2019

Sample Lot Number : 01264712

Number of Sample : 20

Packaging Information : CLOSED PACKED

Expiration Date of the Sample : 10/2024

Production Date of the Sample : 10/2020

Description of the Sample : Powder Free Nitrile Examination Gloves

Characteristics of the Sample

Use/Application : -

Sample Image :



3. TEST SYSTEM

- Animal used in the test** : RABBIT
Strain : NEW ZEALAND
Source : Burdur Mehmet Akif Ersoy University Experimental
Animals Production and Research Center
Gender : FEMALE
Weight : 2000-2300 KG
Age : 6 MONTHS
Acclimation time : 5 DAYS
Number of the animals : 3

4. ANIMAL MANAGEMENT

- Animal Care** : The animals used in the experiments are performed in accordance with the standards of Biological Evaluation of Medical Devices - Part 2: Requirements for Animal Welfare.
- Food** : The SDS brand VRF1 diet is provided as ad-libitum.
- Water** : Water is supplied as ad-libitum in suitable drinkers.
- Cage System** : Each rabbit was identified and placed in appropriate cages.
- Environmental Conditions** : 12 hours night and 12 hours day environment is provided; 30-70% humidity and 16-22°C environment is provided. Temperature and humidity are checked daily.
- Personnel** : Tests are performed by trained and appropriately qualified personnel.
- Selection of the animal** : Healthy, non-disease animals and non-pregnant animals were used under the supervision of a veterinary surgeon.
- Veterinary Care** : This study was carried out under the supervision of a veterinarian.

5. METHOD

Irritation tests were carried out in accordance with ISO 10993-10, care conditions of test animals used in the test, ISO 10993-2, preparation of samples used in the test and reference materials ISO-10993-12.

Test material to be used for irritation tests (specimen) ISO 10993-12 Biological evaluation of medical devices - Part 12: Sample preparation according to the sample preparation and reference materials standard, with 0.2 g / ml sterile 0.9% isotonic in accordance with ISO 10993-12 Prepared at $37 \pm 1^\circ\text{C}$ for 72 ± 2 hours.

As a Positive Control; Sodium Lauryl Sulfate, previously known to have irritant effect.

As Negative Control; Serum Physiological previously known to have no irritant effect.

Irritation tests were performed on 3 healthy, adult Albino rabbits weighing less than 2 kg. Tests were performed by treating the material to be tested directly on the skin as specified in the ISO 10993-10 standard. After shaving enough to provide sufficient application area (10 cm x 15 cm) in the dorsal region of the experimental animals, the samples were applied as shown in Figure 1.

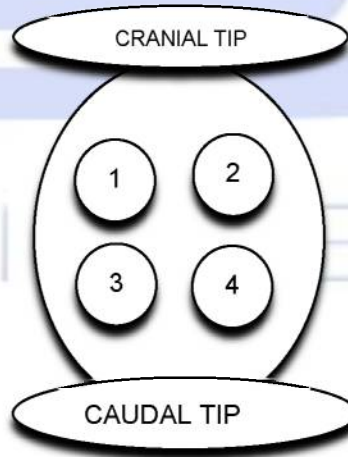


FIGURE 1: Application sides

1. Experimental Side
2. Positive Control
3. Negative Control
4. Experimental Side

6. EVALUATION

The application sites were covered with gauze and then covered with bandage for 4 hours. At the end of the contact period, the dressings were removed and the sites of application were scored for erythema and edema at the 1st hour, 24th hour, 48th hour and 72th hour according to the scoring system given in Table 1 and the irritation index, number (score) and definition in Table 2 (response category).

Table 1. Characteristics of the animals

Animal No	Age	Gender	Weight
1	6 month	Female	2,1 kg
2	6 month	Female	2,3 kg
3	6 month	Female	2,1 kg

Table 2. Scoring system for skin irritation

Reaction	Score
Erythema and eschar formation	
No erythema	0
Very mild erythema (barely visible)	1
Prominent erythema	3
Moderate erythema	2
Grading erythema with severe erythema (red as beet)	4
Edema formation	
No edema	0
Very mild edema	1
Significant edema (the edges of the area of marked edema)	2
Moderate edema (about 1 mm swollen)	3
Severe edema (swelled more than 1 mm and spread out of the exposed area)	4
Total possible score for irritation	8

Other adverse changes in skin locations should be recorded and reported.

The results of the observation following the experiment carried out in accordance with ISO 10993-10 standards are presented in Table 3 and Table 4. Figure 2-9 contains photographs of the test and sample preparation and test application.

After covering the samples with 2.5 cm x 2.5 cm sterile gauze, the whole application area was wrapped with bandage. Samples to be tested for 4 hours were applied to the region. At the end of this period, bandages were opened and samples were taken and the applied areas were marked. The remaining test materials were washed with warm water. After the procedure, the test sites were observed at 1, 24, 48 and 72 hours and samples were evaluated by taking into consideration the criteria specified in Tables 2 and 3.

Table 3. Irritation categories in rabbits.

Mean Score	Irritation category
0 – 0.4	Negligible
0.5 – 1.9	Light
2 – 4.9	Middle
5 - 8	Serious

TEST RESULTS

Table 4. Evaluation scores for the sample.

Animal No	Groups	Application Side	Observation (h)							
			Erythema				Edema			
			1	24	48	72	1	24	48	72
1. Rabbit	Sample	1	0	0	0	0	0	0	0	0
		4	0	0	0	0	0	0	0	0
	Positive Control	2	3	2	1	1	1	2	2	1
	Negative Control	3	0	0	0	0	0	0	0	0
2. Rabbit	Sample	1	0	0	0	0	0	0	0	0
		4	0	0	0	0	0	0	0	0
	Positive Control	2	3	2	1	1	1	2	2	1
	Negative Control	3	0	0	0	0	0	0	0	0
3. Rabbit	Sample	1	0	0	0	0	0	0	0	0
		4	0	0	0	0	0	0	0	0
	Positive Control	2	3	2	2	1	2	2	2	1
	Negative Control	3	0	0	0	0	0	0	0	0

Table 5. Mean score and irritation categories

Groups	Application side	Erythema	Edema	Total	Irritation Category
Sample	2	0	0	0	Negligible
	6	0	0	0	Negligible
Negative Control	3	0	0	0	Negligible
	5	0	0	0	Negligible

7. RESULT

As mentioned above, after the observations at the three time points for the two criteria (Table 3), overall mean scores were obtained by averaging the scores for the test material (Table 4). In the observations of the tested material, in any application sites and injection points, erythema and edema formations were not observed. According to the data obtained from observations and the evaluation criteria defined in the ISO 10993:10-2010, the tested sample defined as the sample has no irritation effect.

8. RECORD

All raw data and a copy of the final report are stored in the Medicert archive files.

9. REFERENCES

- Guide For The Care And Use Of Laboratory Animals Eighth Edition National Research Council of The National Academies
- TS EN ISO 10993-1 Biological evaluation of Medical Devices - Chapter 1: Evaluation and experiment in a risk management process
- TS EN ISO 10993-2 Biological evaluation of Medical Devices – Chapter 2: Conditions for animal welfare
- TS EN ISO 10993-10 Biological evaluation of Medical Devices – Chapter 10: Experiments for irritation and skin sensitivity
- TS EN ISO 10993-12 Biological evaluation of Medical Devices – Chapter 12: Sample preparation and reference materials